

AR006076 • AR004175 • AR006077 • AR004090 • AR006079 • AR005169 • AR006080

PRODUCT DESCRIPTION

The dataloggers Uxxxx with connectors for external probes connection are designed for measuring and recording physical and electric quantities with an adjustable logging interval from 1 second to 24 hours. The measured values, or the average values and min/max values over a recording interval are stored into the internal non-volatile memory. The data logging mode can be cyclic (when the data memory is completely full, the oldest data are overwrite by the new ones), or non-cyclic (the recording will stop once the memory is full). The device also allows to the evaluation of alarm states - exceeding the limit of the measured value or falling below this limit, exceeding the limit of memory filling, technical defects of the instrument or probes. The alarm signalling can be realised visually, optionally by a symbol appearing on the display or by a short blink of an LED, or acoustically. The data recording can be performed continuously or only when an alarm occurs. The devices are powered by internal a replaceable lithium battery (AR006079 is powered by internal Li-Ion accu-pack). **Device setting, recorded data downloading and online monitoring** is carried out using the computer with the software installed see www.guilcor.com. The USB interface is used to communicate with the computer.

Device type	Measured values	Construction
AR006076	Te	Connector for external Pt1000/E probe connection
AR004175	2 x Te	Connectors for up to four external Pt1000/E probe connection
AR006077	Ti + Te	Internal temperature sensor and connector for external Pt1000/E probe connection
AR004090	4 x Te	Connectors for up to four external Pt1000/E probe connection
AR006079	P + CO ₂	Internal barometric pressure sensor and connector for external CO ₂ probe connection
AR005169	Te + RH + Td	Connector for Digi/E probe connection
AR006080	Ti + Te + RH + Td	Internal temperature/humidity sensor and connector for external Pt1000/E probe connection

Ti ... Internal temperature, Te...External temperature, RH...Relative humidity, P... Barometric pressure, Td...Dew point temperature

INSTALLATION AND OPERATION

Fasten the device on the wall with two screws or insert it into the wall holder **LP100** (optional accessory). Working position of the device is arbitrary with the exception of the AR006080, which place the USB connector facing down. Dataloggers can also be operated as a portable, in this case protect them from falling and try to adhere to the working position.

- Please pay attention to the device and probes mounting. Inappropriate selection of the working position and the measurement location may adversely affect the accuracy and long-term stability of the measured values.
- Connect the probes to the device (maximum cable length of the Digi/E probe should not exceed 30 m, recommended maximum cable length of the Pt1000/E probe is 15 m, maximum cable length of the CO₂ probe is 4 m)
- The devices with all cables should be located as far as possible from potential interference sources

Set-up the device

- Device setup can be performed using the computer with the Windows 7 operational system or higher. Minimum HW requirements are 1.4 GHz processor and 1 GB memory.
- Install the software into computer (the program is available free of charge at www.guilcor.com)
- Connect the datalogger to the computer. Use an USB cable with USB-C connector (max. cable length 3 m).
- Click on the **Configuration** button. The device configuration will be downloaded and you can change the settings of some items
- Save the new configuration into the device and disconnect the device from the computer (close USB connector with a closing cap)

Operating the device from the keypad

- Press and hold the lower key. After the light up the row with menu items, release the key and briefly press the upper key.
- Press the upper key to scroll through the menu items (device turning On/Off, deleting the Min/Max values in the device, ...)
- Press the lower key to confirm (SET)

The devices do not require special maintenance. We recommend that you regularly verify the accuracy of the measurement with calibration.




SAFETY INSTRUCTIONS



- Installation, electrical connection and commissioning should only be performed by qualified personnel in accordance with applicable regulations and standards
- The datalogger **AR006079** is equipped with an internal **Li-Ion accumulator**. Observe the recommended operating and storage condition. Should the battery casing get damaged or should the whole device get destroyed, carry it outside the fire, high temperature or water affected area to a safe fire-protected place. Protect yourself and the environment against escaping gases and against being soiled with the battery electrolyte.
- The accumulator charging of the **AR006079** device will proceed at an indoor temperature ranging between 0° C and +40°C (the device has to be located in an indoor room with a relative humidity up to 85%)
- Devices contain electronic components, it needs to liquidate them according to currently valid conditions.
- To **complement the information in this data sheet** read the manuals and other documentation, which are available in the **Download** section for a particular device at www.guilcor.com

Technical specifications

Device type	AR006076	AR004175	AR004090	AR006077	AR005169	AR006080	AR006079
Power batteries	Lithium battery 3.6 V	Lithium battery 3.6 V	Lithium battery 3.6 V	Lithium battery 3.6 V	Lithium battery 3.6 V	Lithium battery 3.6 V	Li-Ion accu pack 3,6V
Recording interval	(1 - 2 - 5 - 10 - 15 - 30) s • (1 - 2 - 5 - 10 - 15 - 30) min. • (1 - 2 - 3 - 4 - 6 - 8 - 12 - 24) h						
Memory capacity	500 000 values in non-cyclic record mode • 350 000 values in cyclic record mode						
Internal temperature measuring range				-30 to +70°C		-30 to +70°C	
Accuracy of internal temperature measurement				± 0.4°C		± 0.4°C	
External temperature measuring range	-90 to +260°C	-200 to +260°C	-200 to +260°C	-90 to +260°C	according to the probe	-90 to +260°C	
Accuracy of external temperature measurement	± 0.2°C *	± 0.2°C *	± 0.2°C *	± 0.2°C *	according to the probe	± 0.2°C *	
Relative humidity measuring range (without condensation)					according to the probe	0 to 100 %RH	
Accuracy of relative humidity sensor					according to the probe	± 1.8 %RH **	
Dew point temperature measuring range					according to the probe	-60 to +70 °C	
Accuracy of dew point temperature measurement					according to the probe	± 1.5 °C ***	
Barometric pressure measuring range							700 to 1100 hPa
Accuracy of barometric pressure measurement at 23°C							± 1.3 hPa
Range and accuracy of CO2 concentration measurement							according to the probe
Recommended calibration interval	2 years	2 years	2 years	2 years	according to the probe	1 year	1 year
Protection class - case with electronics / CO2 probe / T+RH sensor	IP67 / — / —	IP67 / — / —	IP67 / — / —	IP67 / — / —	IP67 / — / —	IP67 / — / IP30	IP54 / IP65 / —
Temperature operating range of the case with electronics	-30 to +70°C	-30 to +70°C	-30 to +70°C	-30 to +70°C	-30 to +70°C	-30 to +70°C	-30 to +70°C
Temperature operating range of the external CO2 probe							-20 to +60°C
Relative humidity operating range (without condensation)	0 to 100%RH	0 to 100%RH	0 to 100%RH	0 to 100%RH	0 to 100%RH	0 to 100%RH	0 to 100%RH
Recommended storage temperature	-20 to +45°C	-20 to +45°C	-20 to +45°C	-20 to +45°C	-20 to +45°C	-20 to +45°C	-20 to +45°C
Recommended storage relative humidity	5 to 90 %RH	5 to 90 %RH	5 to 90 %RH	5 to 90 %RH	5 to 90 %RH	5 to 90 %RH	5 to 90 %RH
Electromagnetic compatibility according to	EN 61326-1	EN 61326-1	EN 61326-1	EN 61326-1	EN 61326-1	EN 61326-1	EN 61326-1
Weight (without the probes)	120 g	120 g	130 g	120 g	120 g	130 g	260 g
Dimensions [mm]							

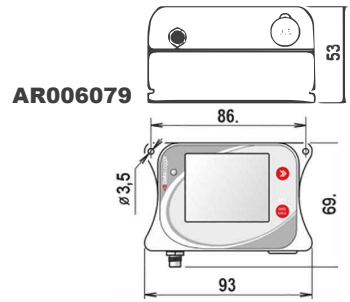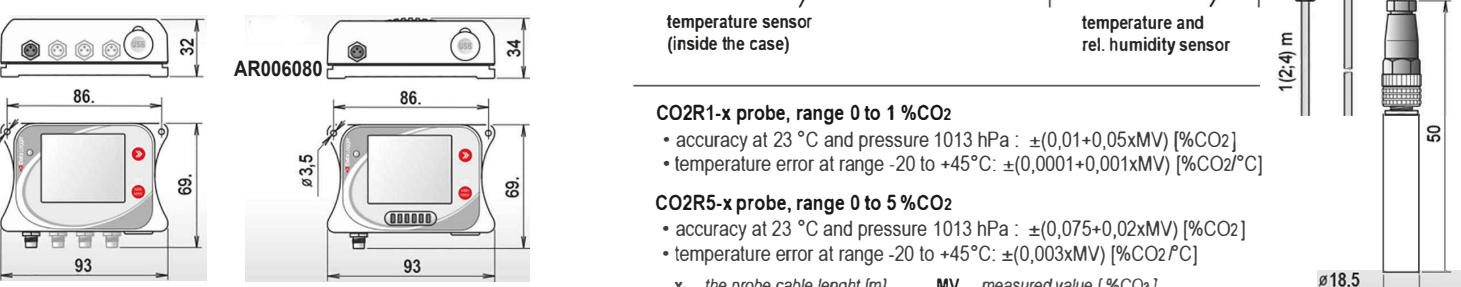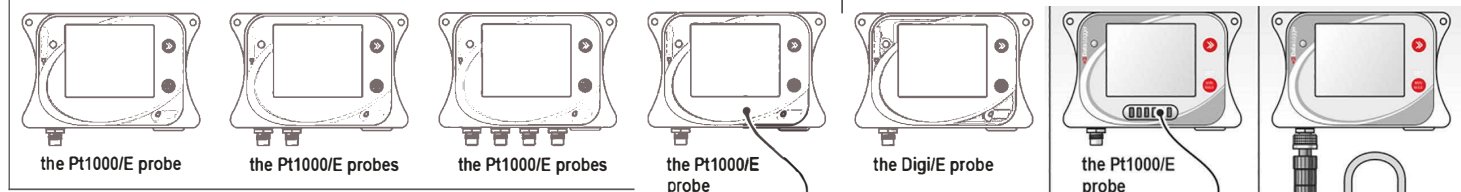

AR006076
AR004175
AR006077
AR004090
AR005169

AR006080

temperature sensor (inside the case)

temperature and rel. humidity sensor


CO2R1-x probe, range 0 to 1 %CO2

- accuracy at 23 °C and pressure 1013 hPa : ±(0,01+0,05xMV) [%CO2]
- temperature error at range -20 to +45°C: ±(0,0001+0,001xMV) [%CO2/°C]

CO2R5-x probe, range 0 to 5 %CO2

- accuracy at 23 °C and pressure 1013 hPa : ±(0,075+0,02xMV) [%CO2]
- temperature error at range -20 to +45°C: ±(0,003xMV) [%CO2/°C]

x ... the probe cable lenght [m] MV ... measured value [%CO2]



* the accuracy of the device without probe in the range to +100 °C (in the temperature range of +100 to +260 °C is accuracy ±0,2 % of measured value)
** at temperature 23 °C in the range of 0 to 90 %RH (hysteresis ±1 %RH, non-linearity ±1 %RH, temperature error 0.05 %RH/°C at 0 to 60 °C)

*** at ambient temperature T < 25°C and RH> 30 %RH (for more details see graphs at device manual)